

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

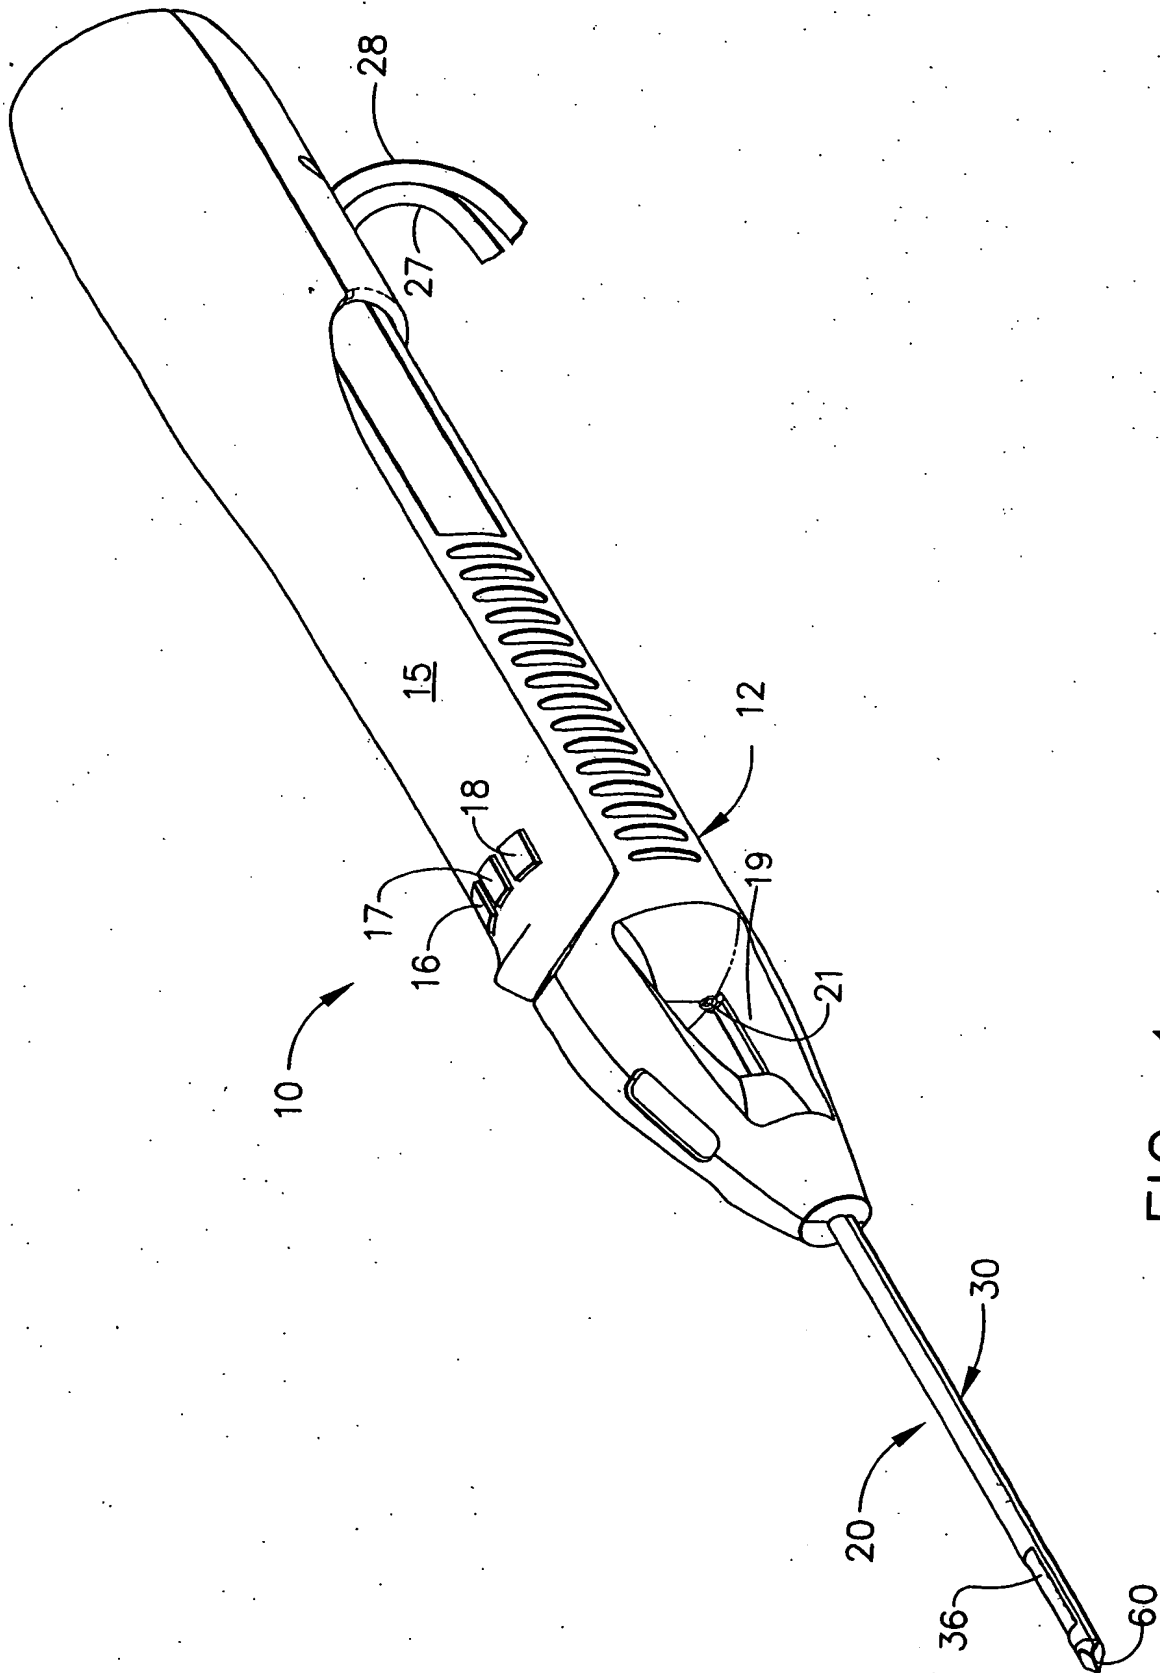

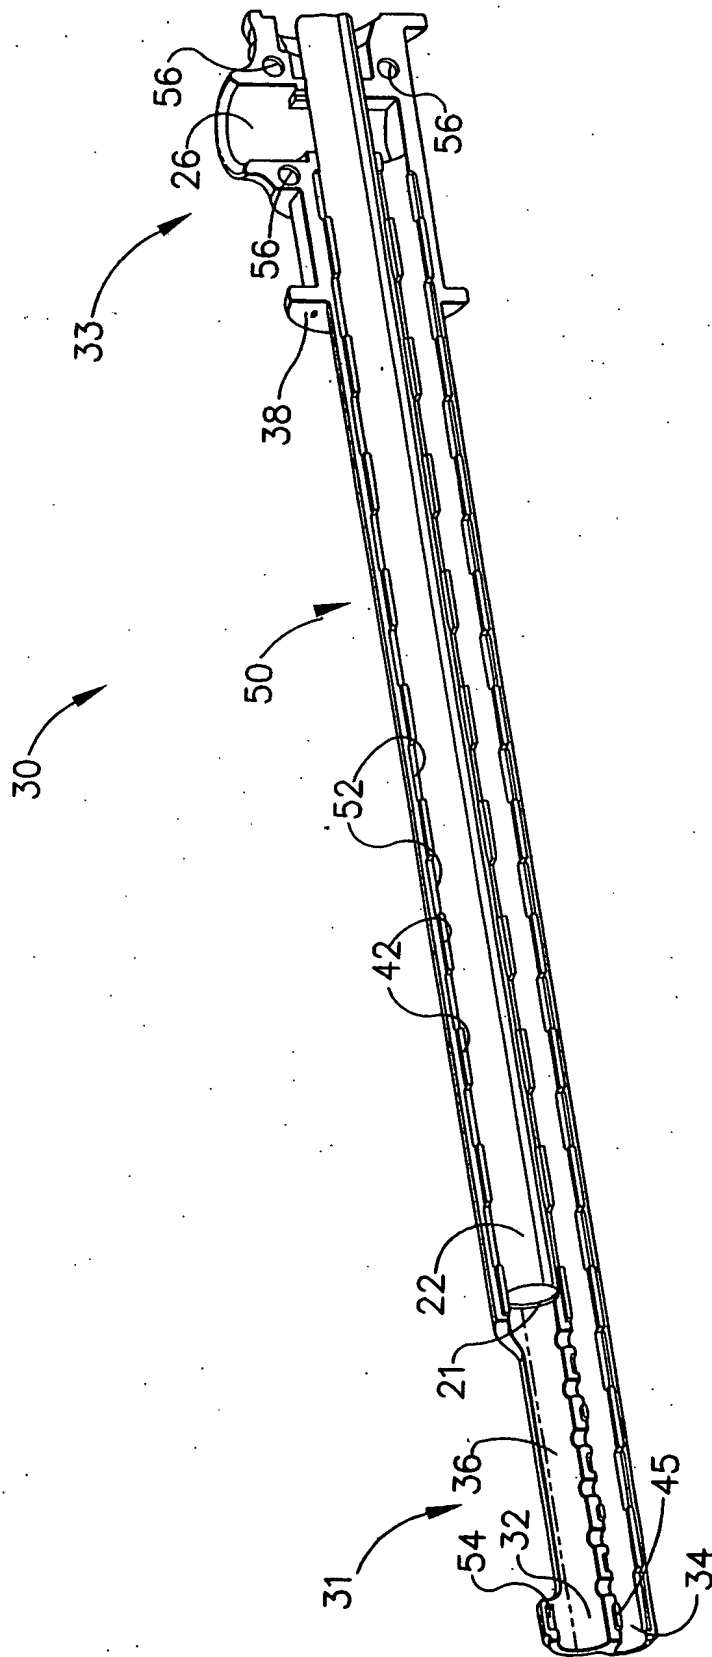


FIG. 1

ATTY: Gerry Gressel Phone: (513) 337-3535  
Customer Number: 000027777





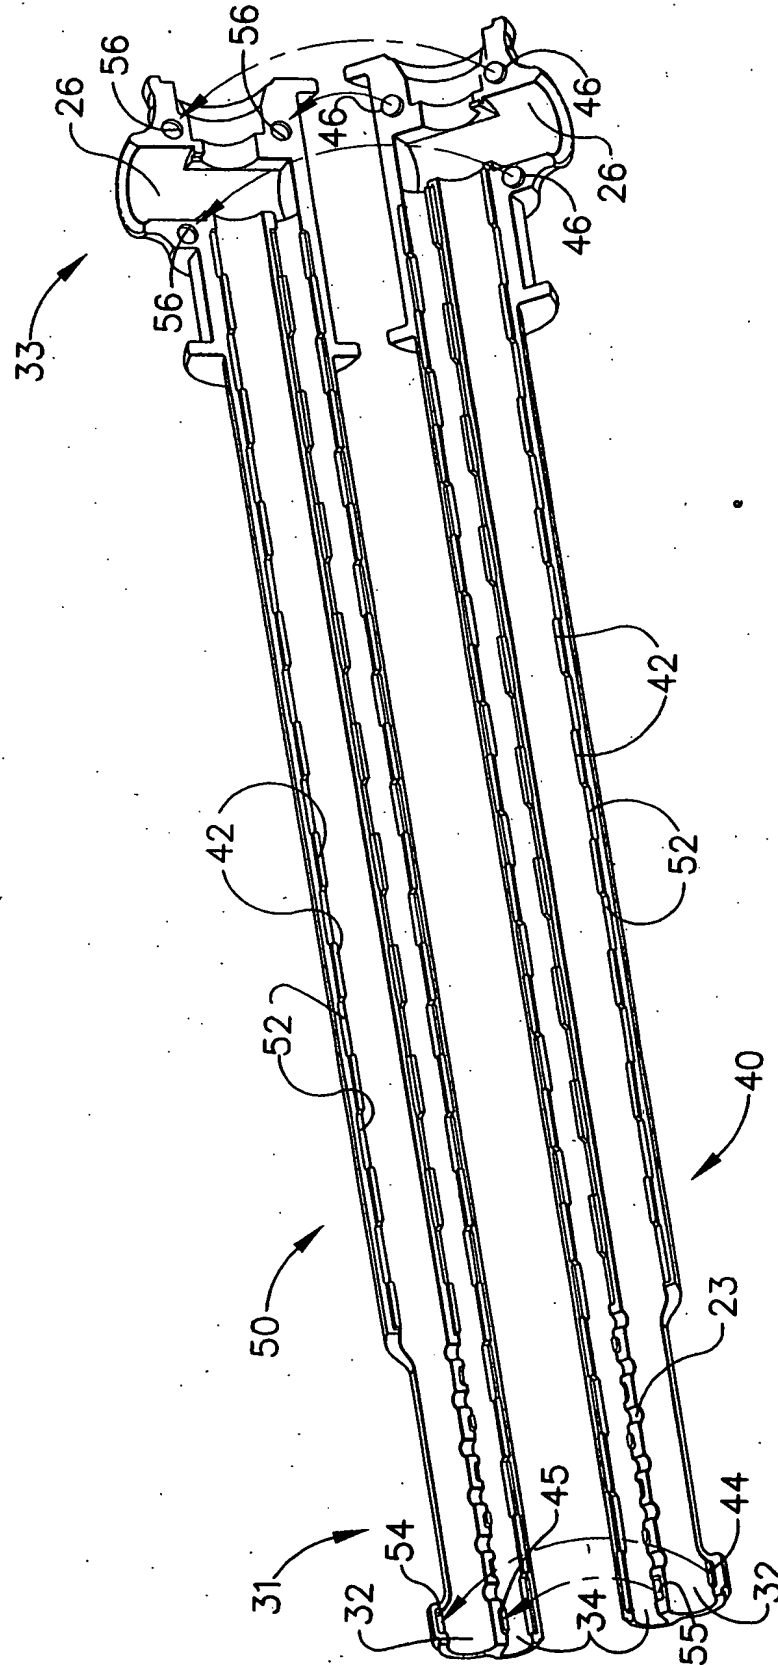


FIG. 4

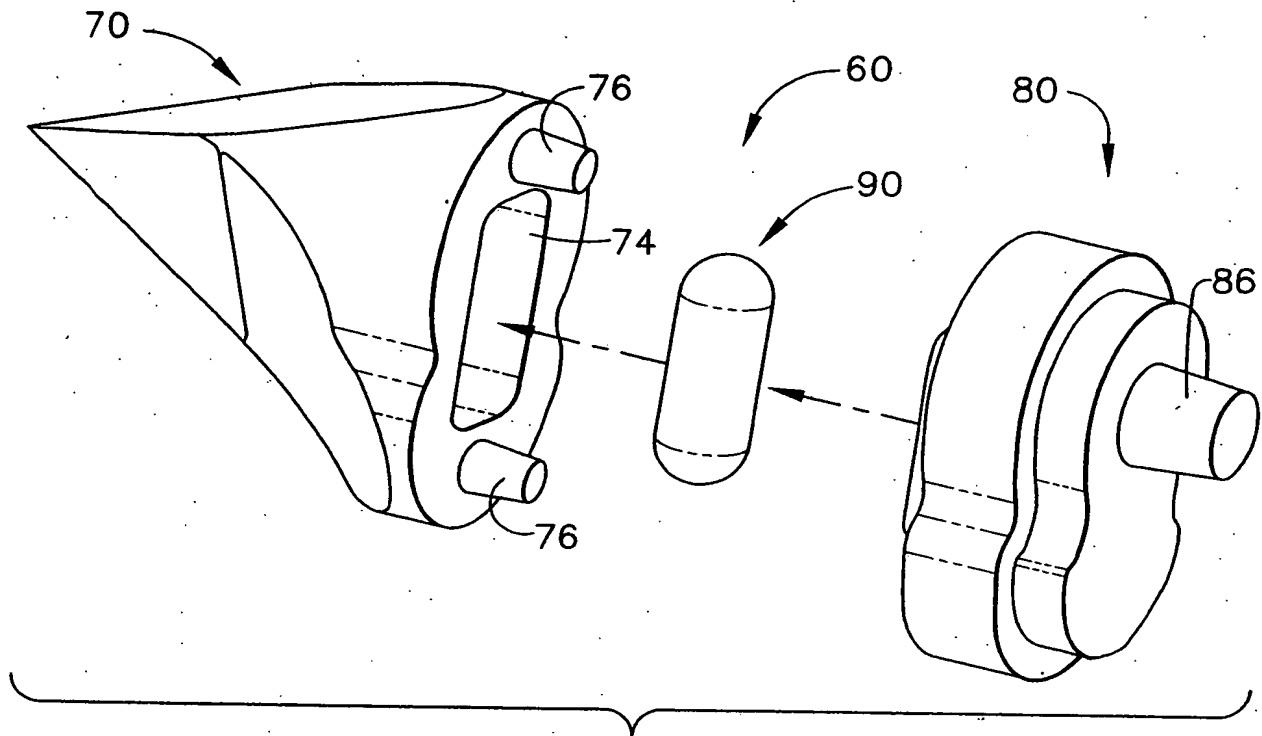


FIG. 5

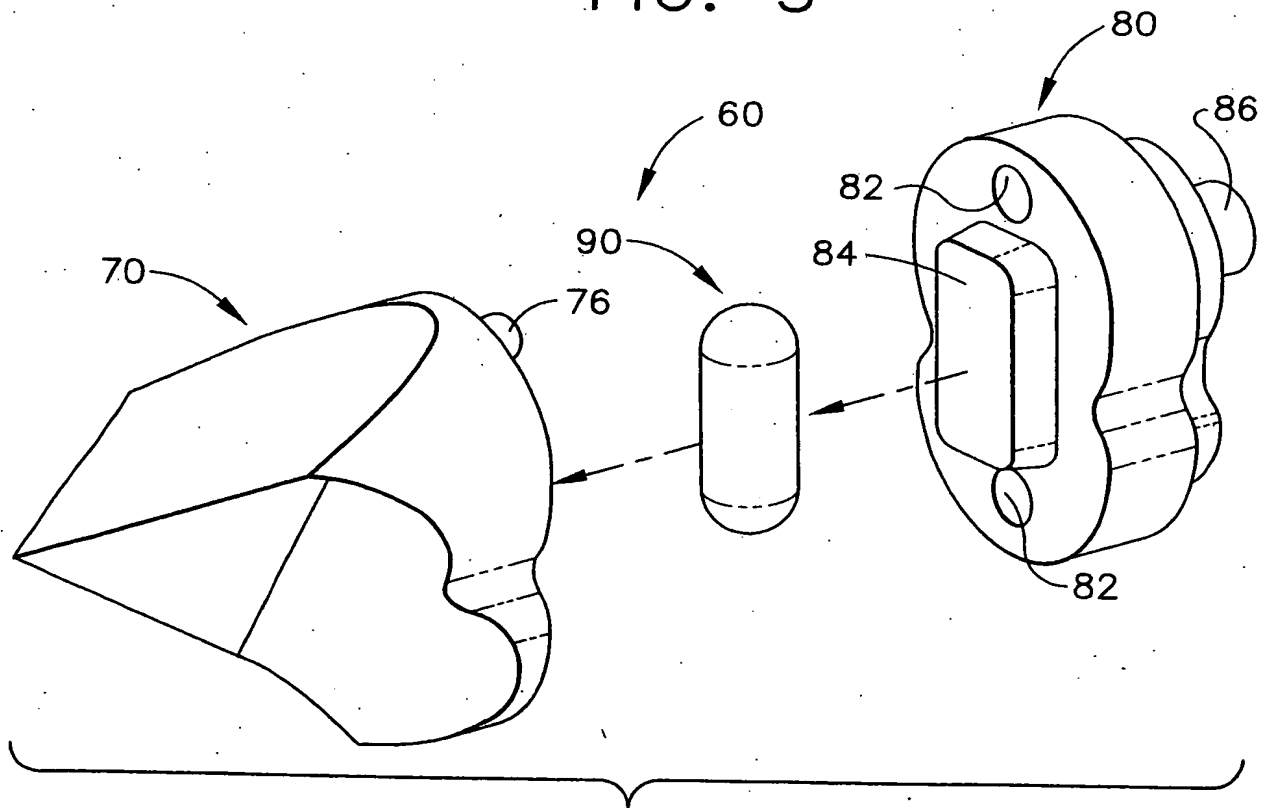


FIG. 6

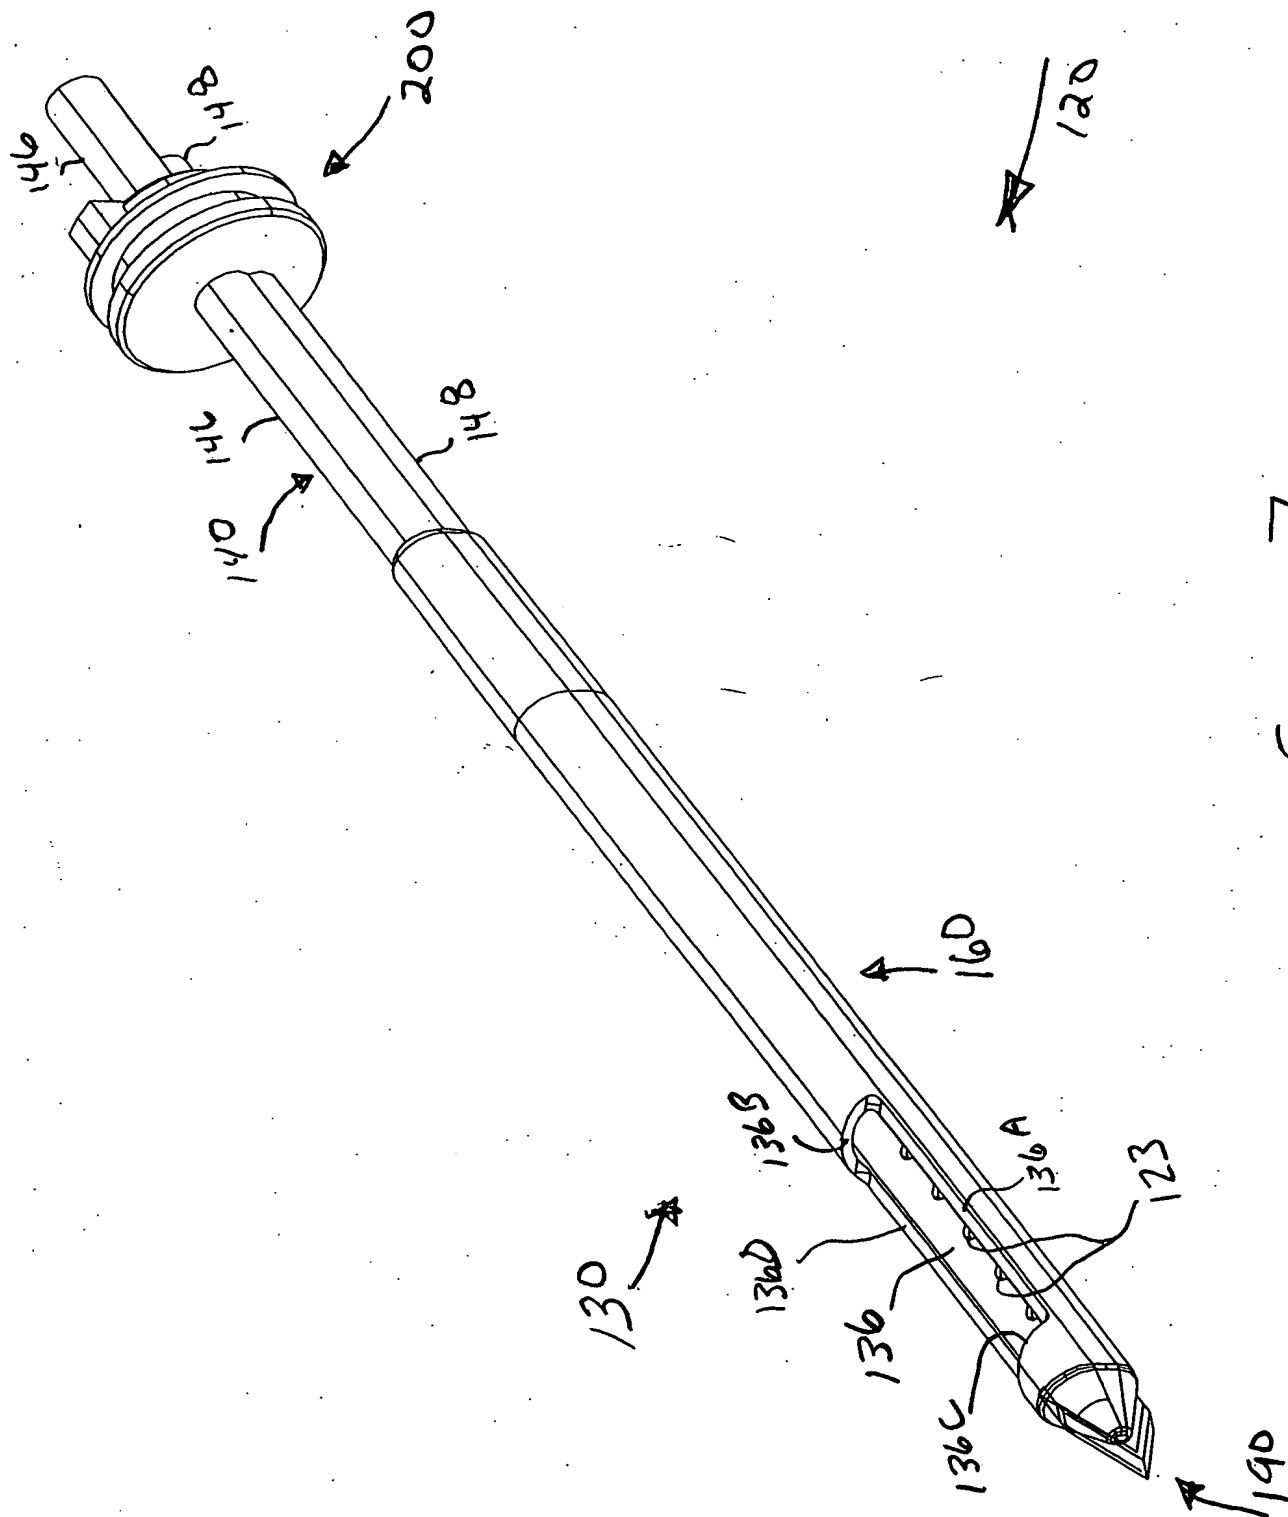


Figure 7

Title: BIOPSY DEVICE  
Inventor: Mark Tsonton et al.  
Docket: END-5293  
ATTY: Gerry Gressel Phone: (513) 337-3535  
Customer Number: 000027777

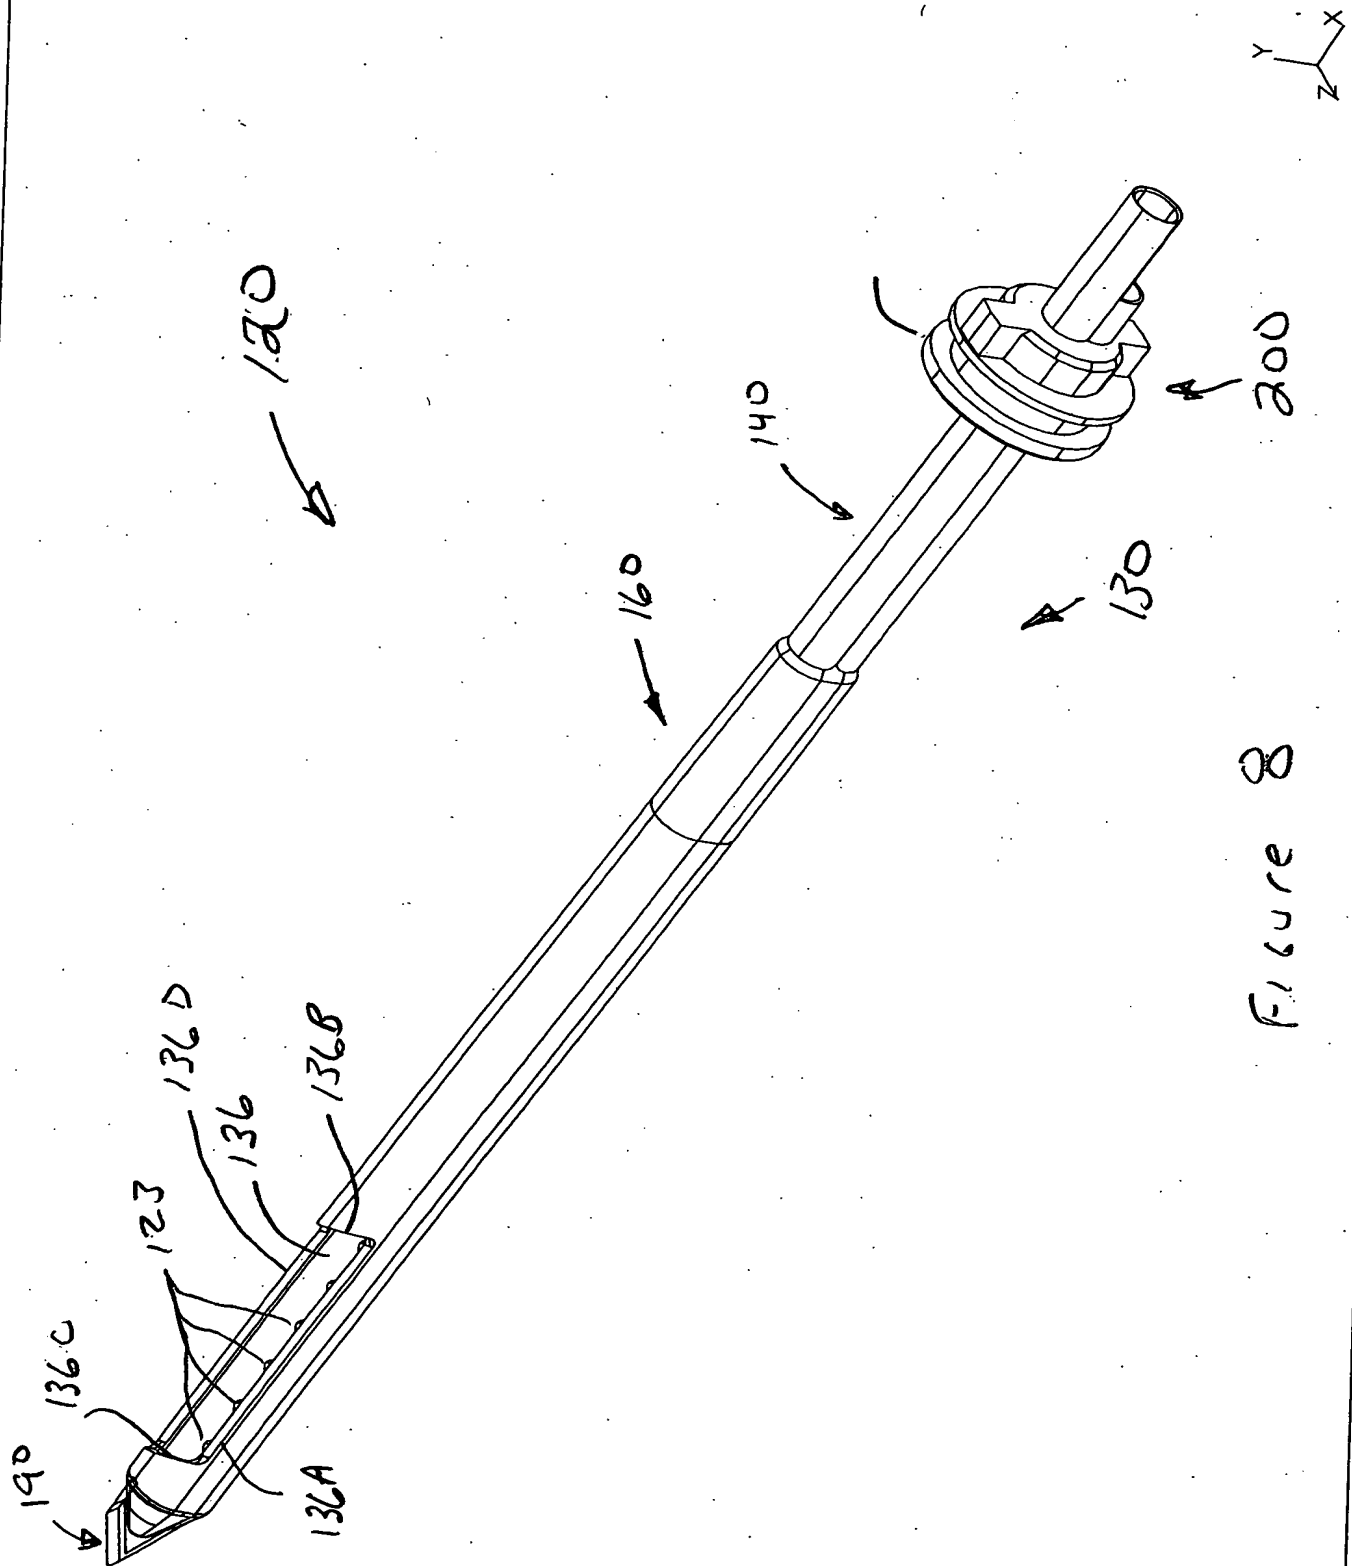


Figure 8



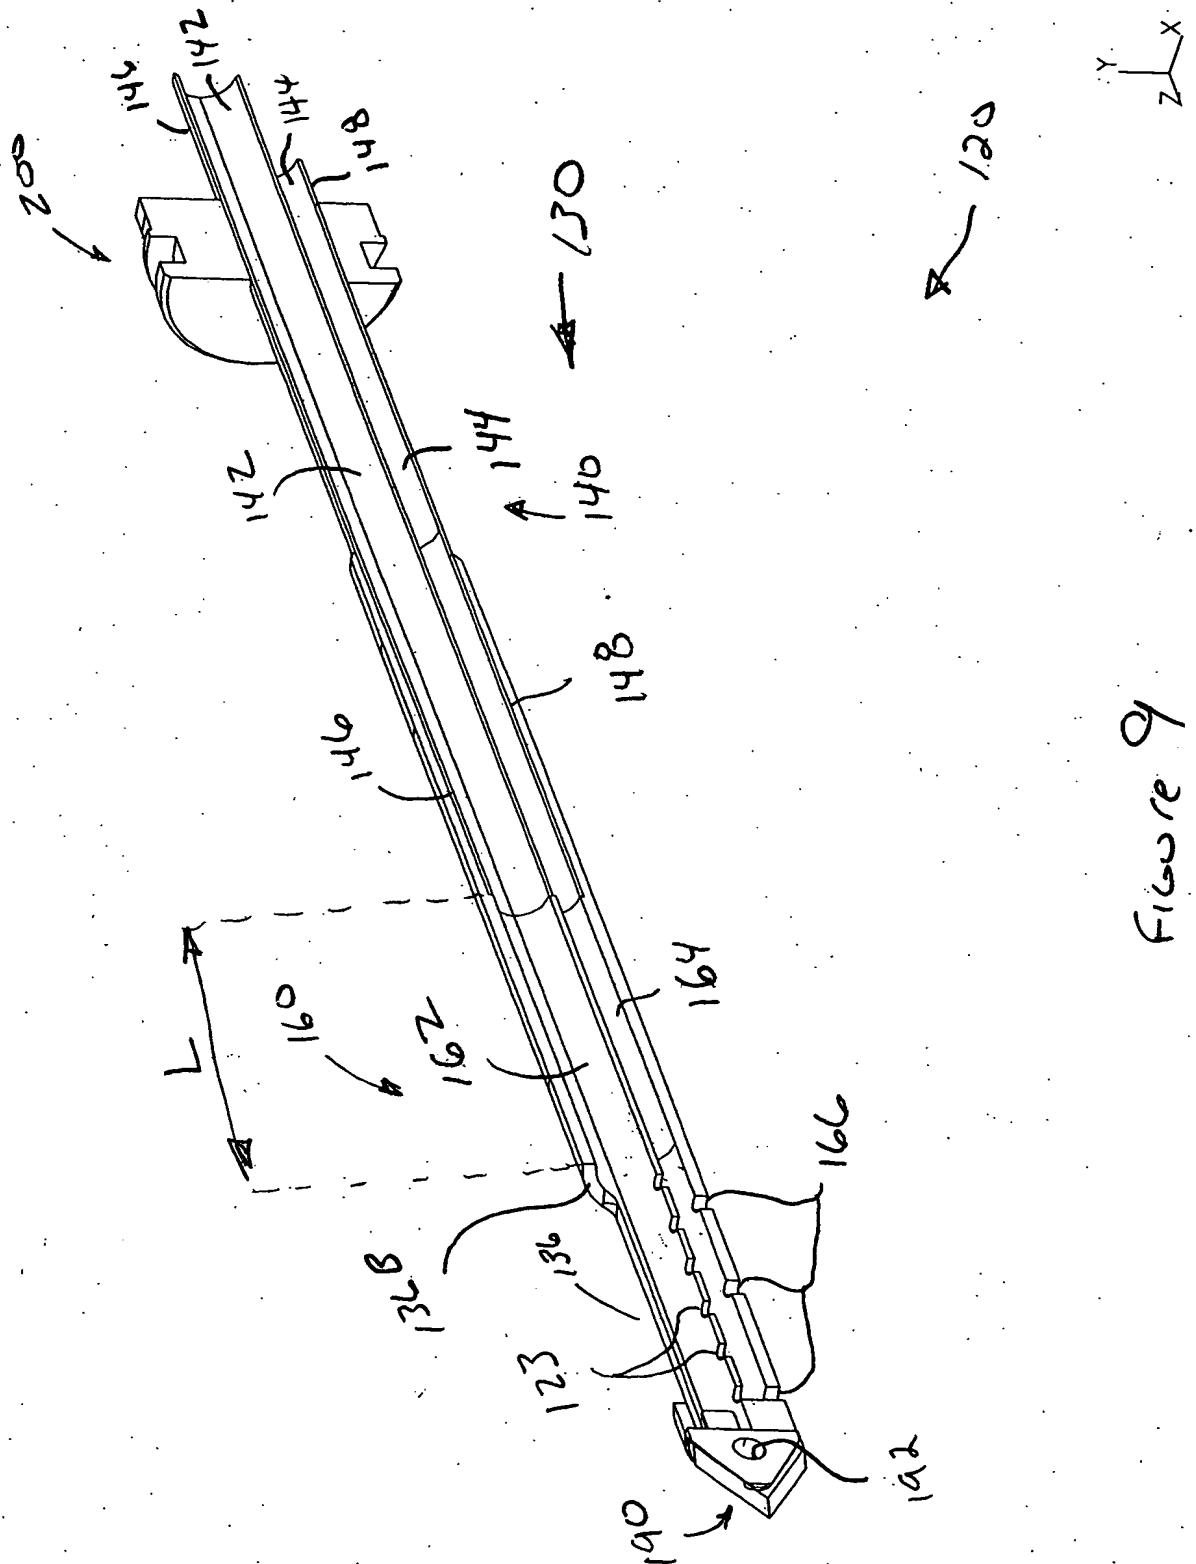


Figure 9

Title: BIOPSY DEVICE  
Inventor: Mark Tsonton et al.  
Docket: END-5293  
ATTY: Gerry Gressel Phone: (513) 337-3535  
Customer Number: 000027777

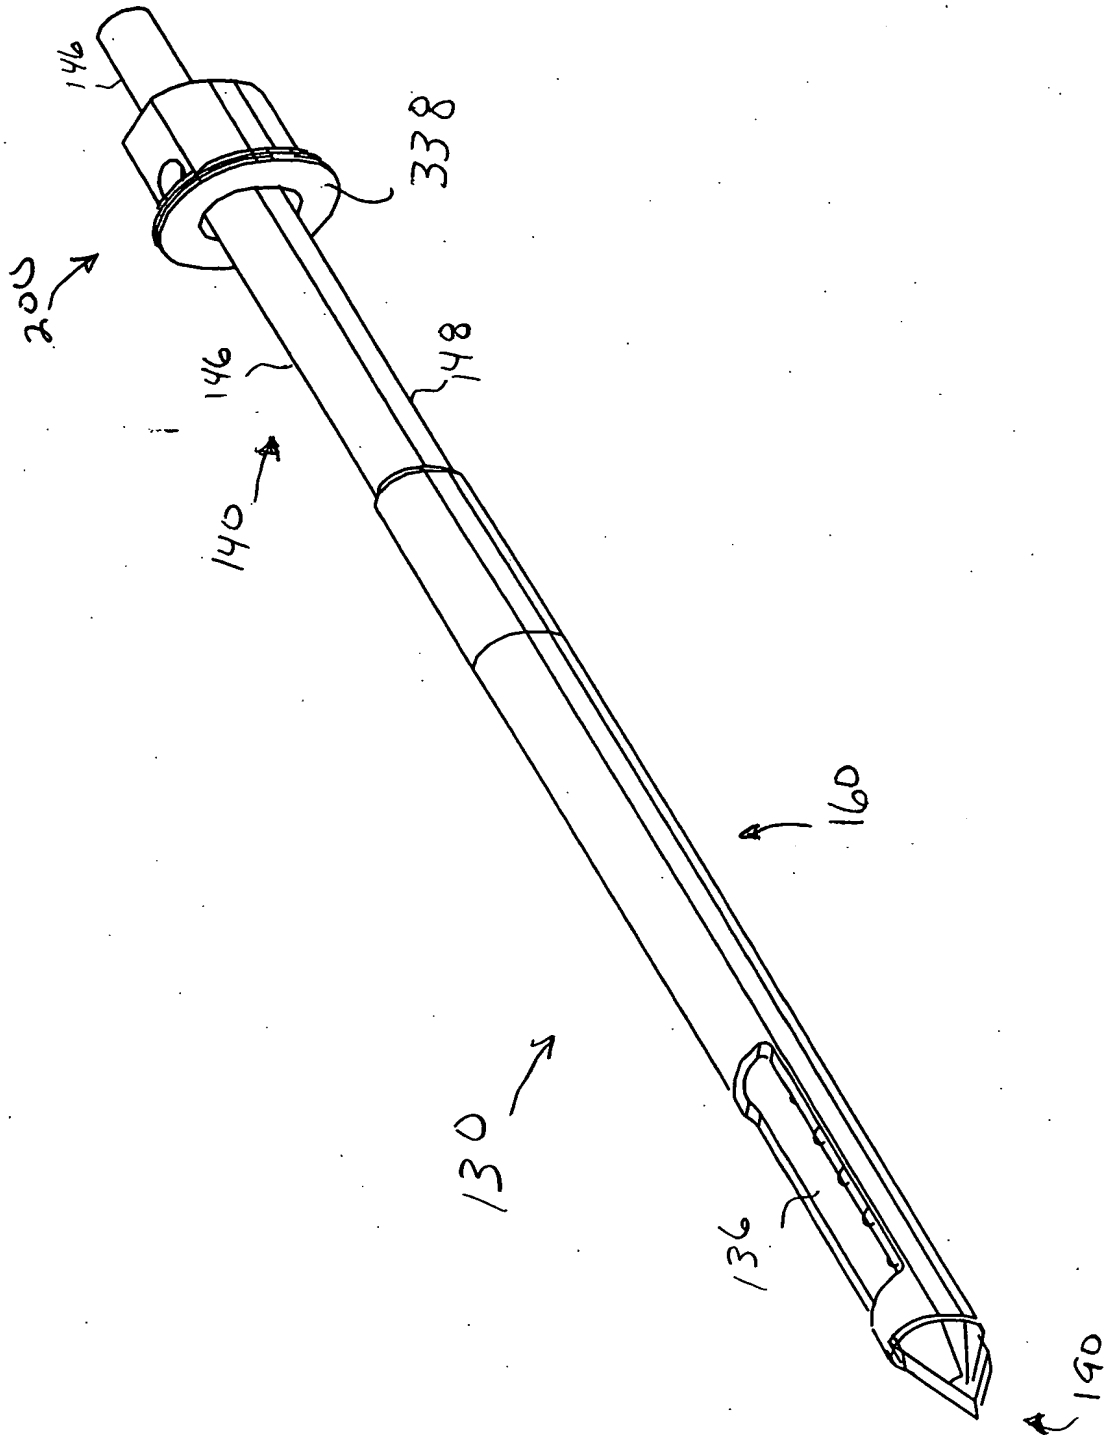


Figure 10

Title: BIOPSY DEVICE  
Inventor: Mark Tsonton et al.  
Docket: END-5293  
ATTY: Gerry Gressel Phone: (513) 337-3535  
Customer Number: 000027777

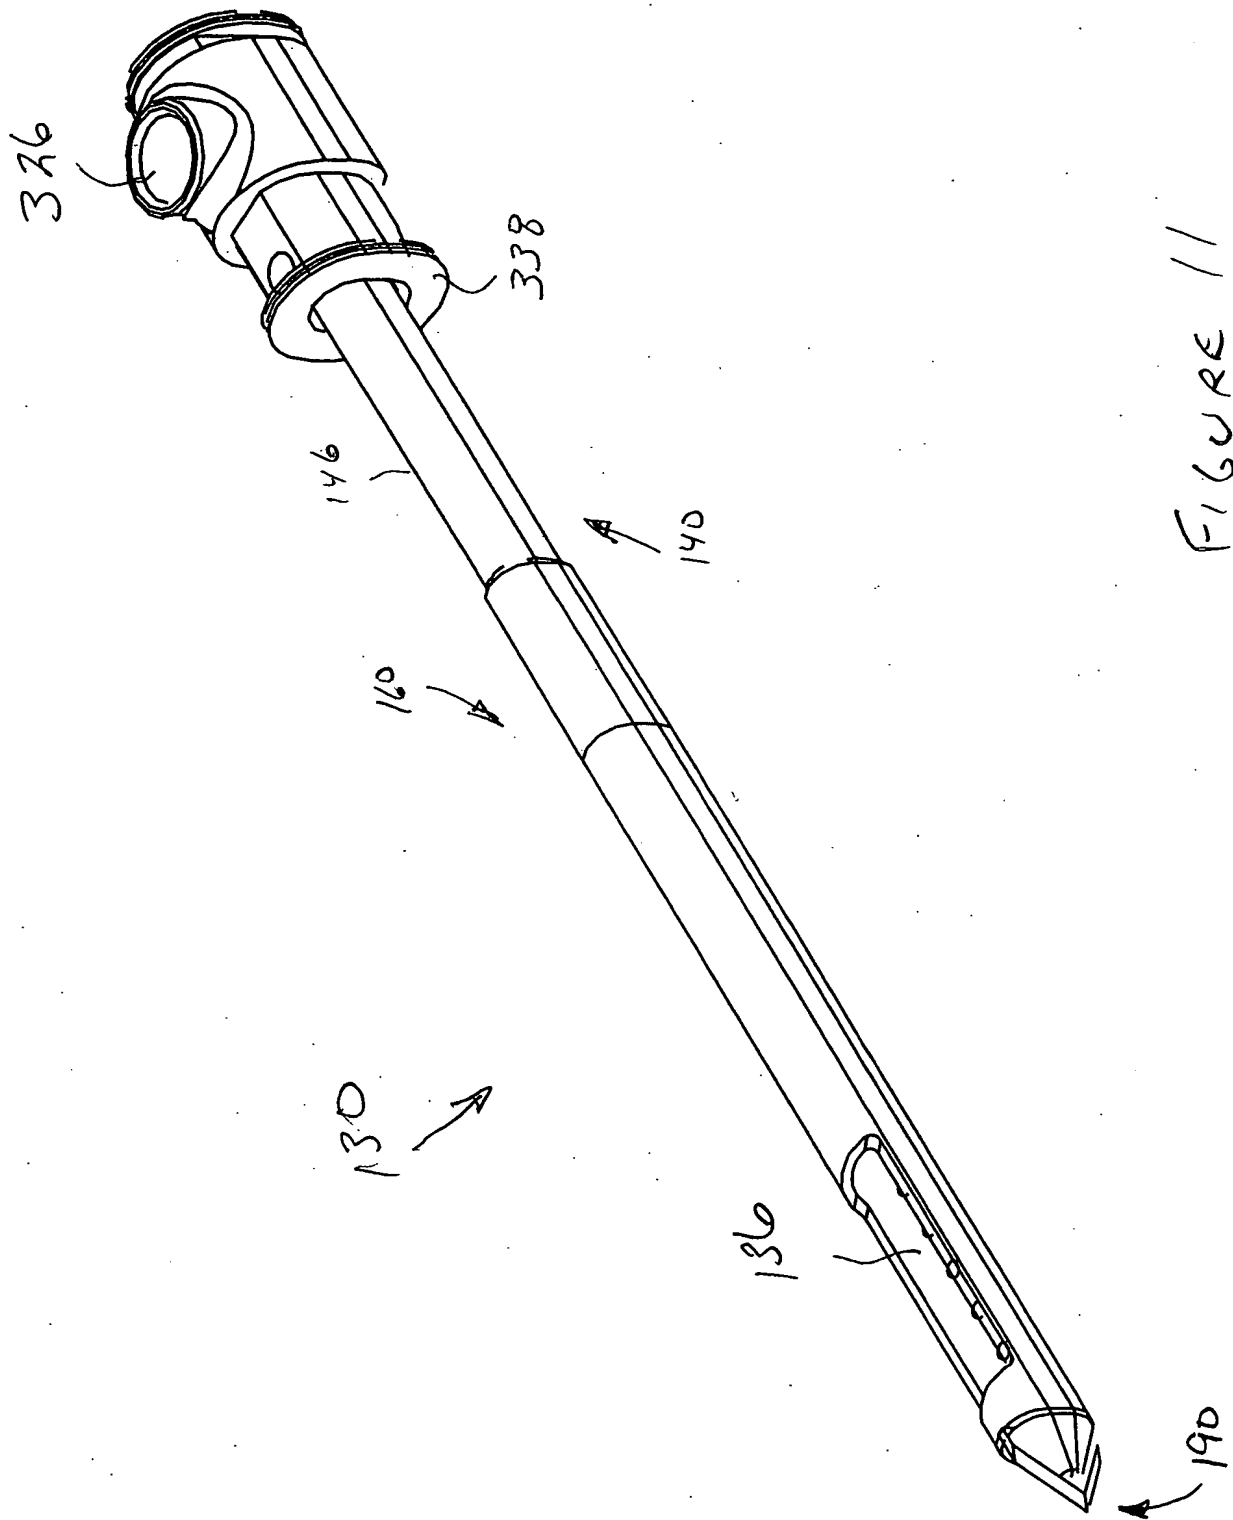


FIGURE 11

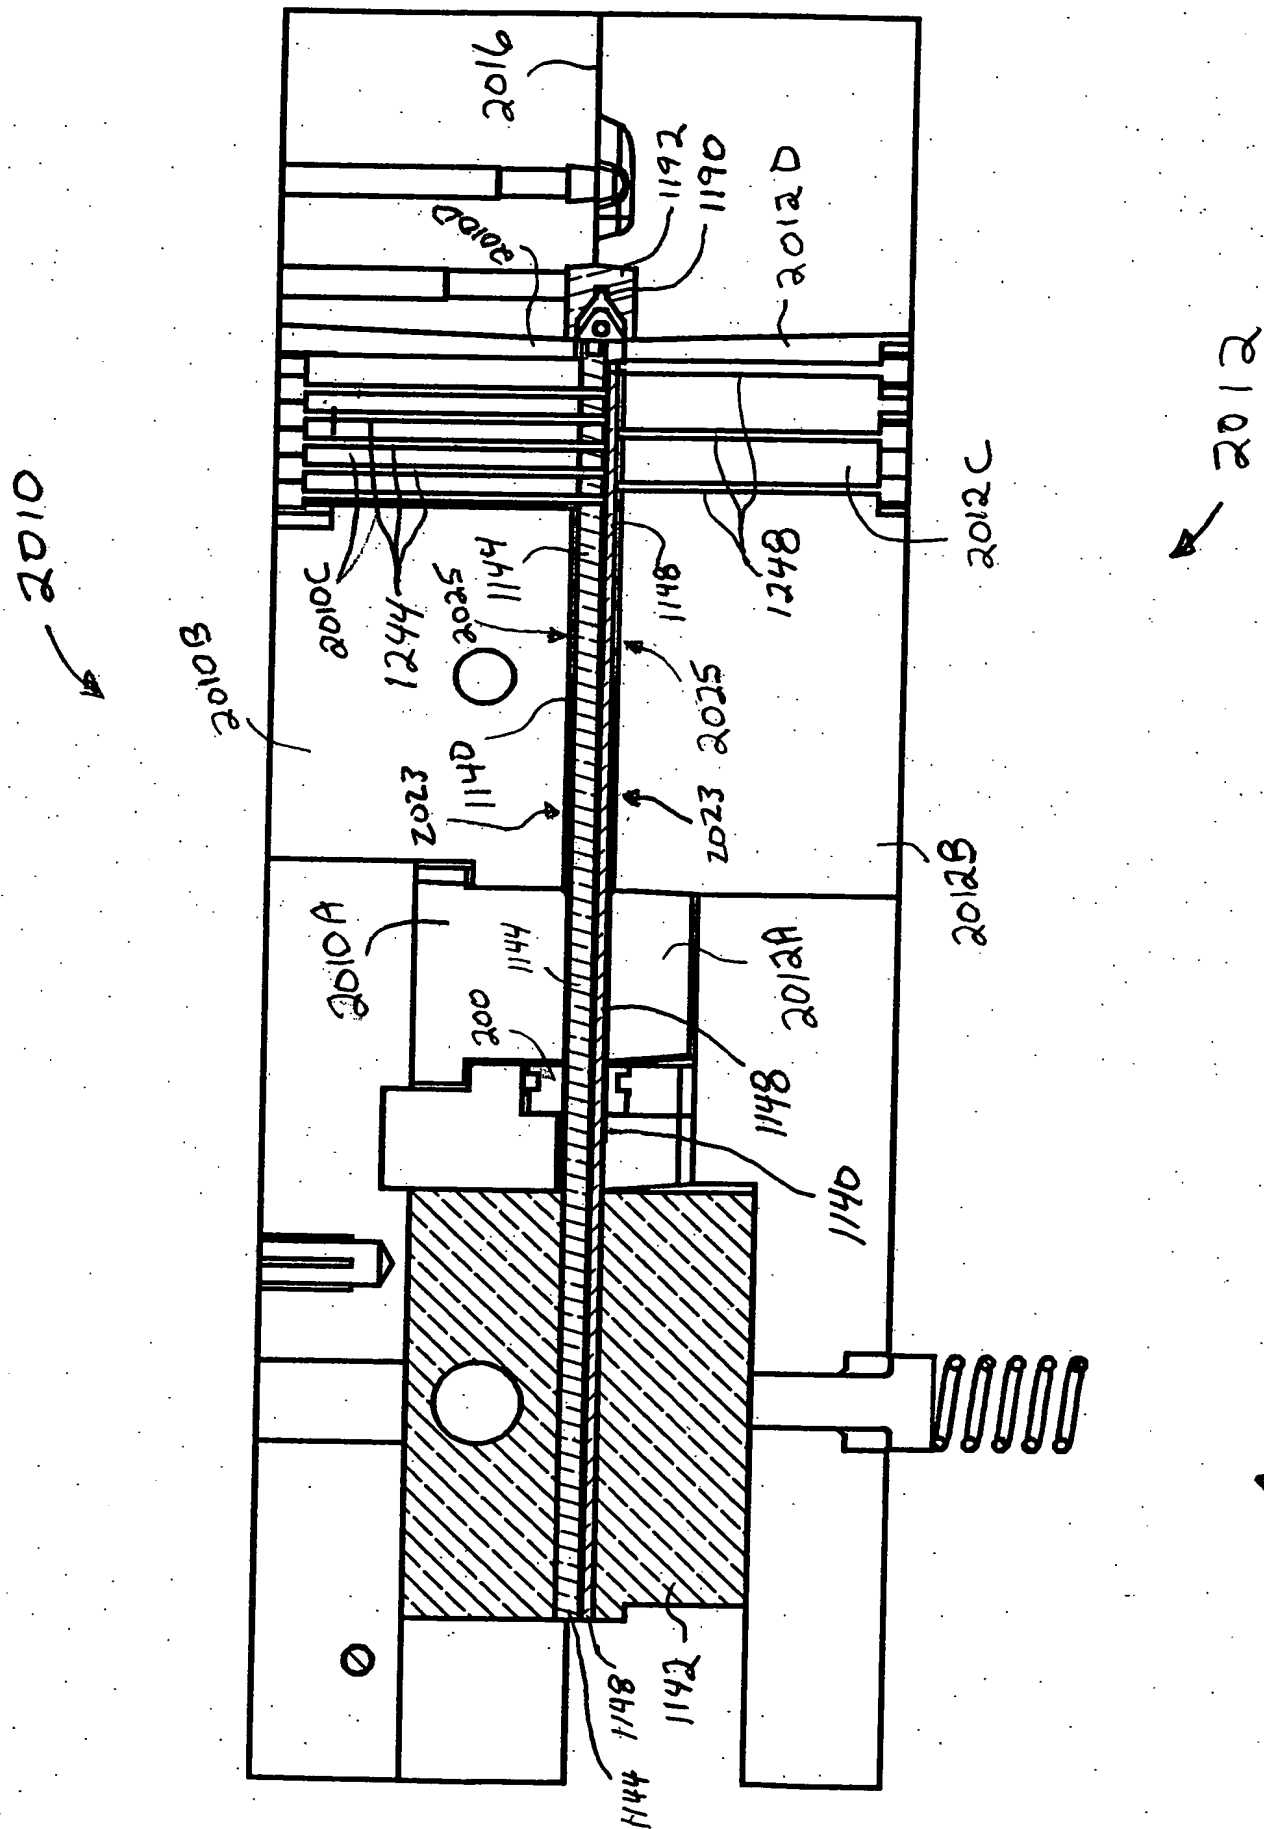


FIG 12  
 FIG 12

2000